


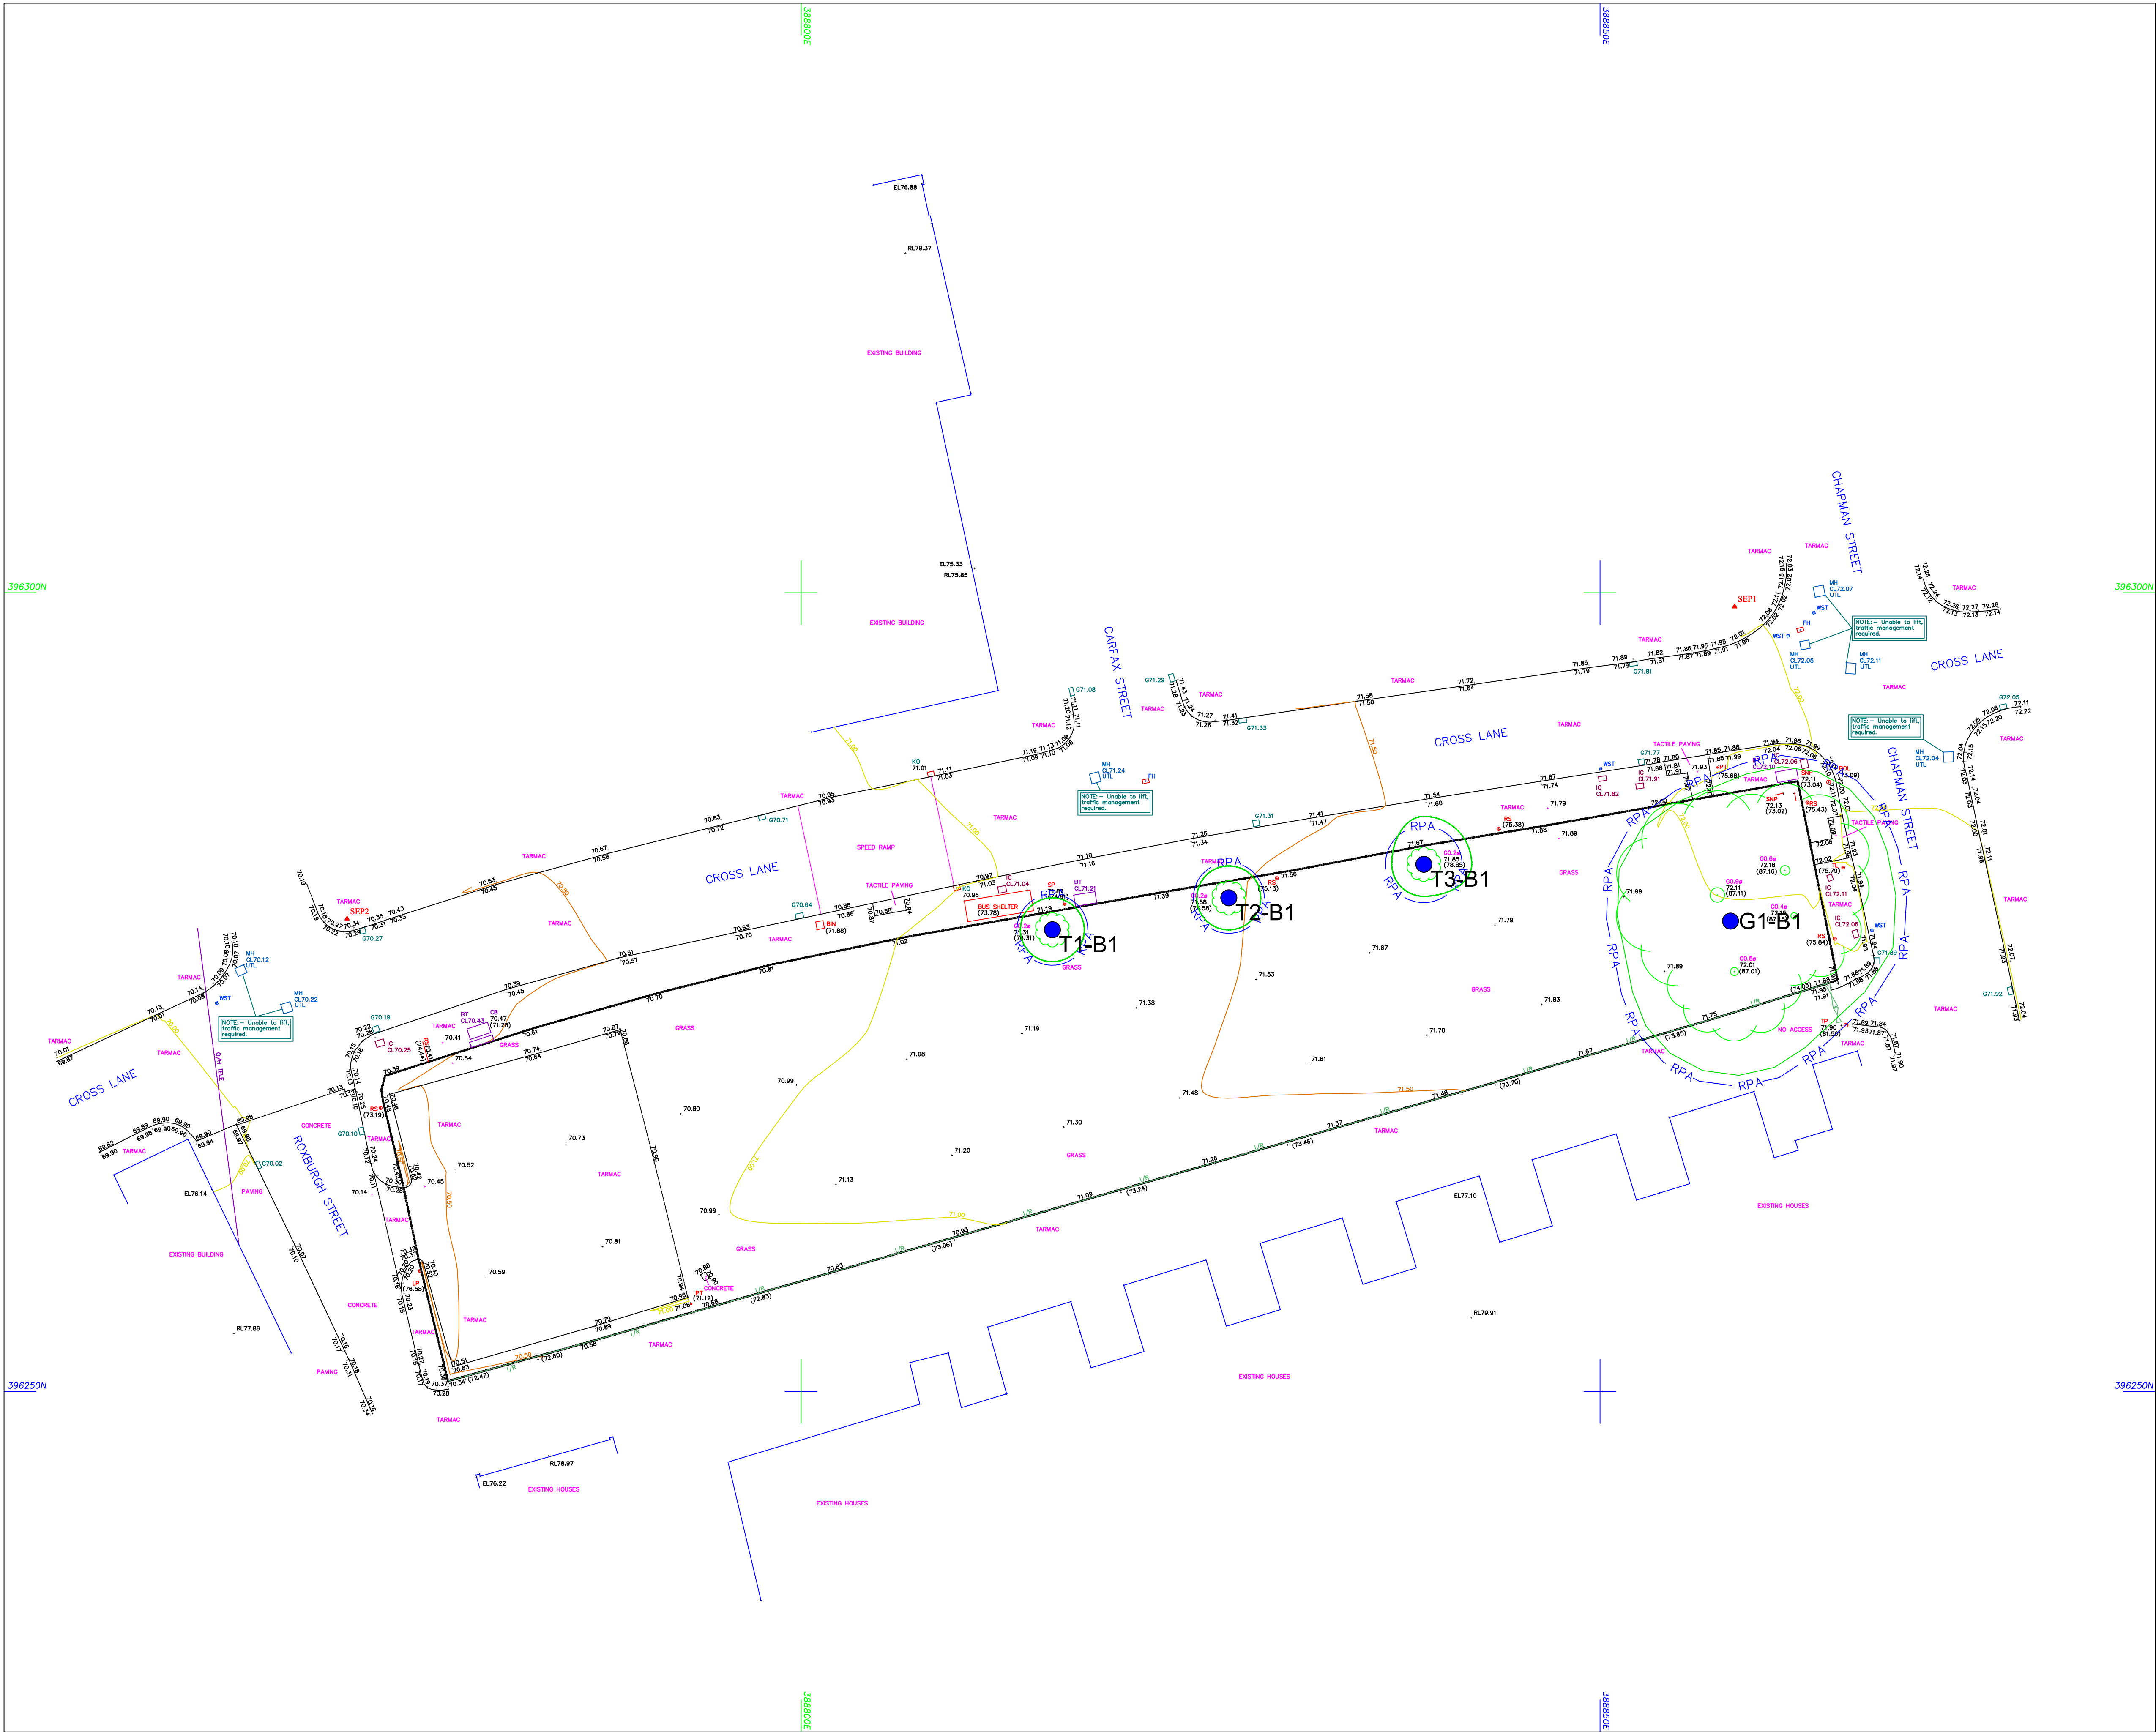

© ACS Consulting

A0

The survey has been prepared at the survey grade indicated below with its accuracy commensurate with the intended scale and purpose. It is not to be used for any other purpose. The survey is not to be used for any other purpose. The survey is not to be used for any other purpose.

It is the responsibility of the client to ensure that the survey is used for the intended purpose. The survey is not to be used for any other purpose. The survey is not to be used for any other purpose.

It is the responsibility of the client to ensure that the survey is used for the intended purpose. The survey is not to be used for any other purpose. The survey is not to be used for any other purpose.

Arboricultural Legend

INDIVIDUAL TREE

INDICATIVE EXTENT OF GROUPED FEATURE

CATEGORY GRADE A  
Trees of high quality

CATEGORY GRADE B  
Trees of moderate quality

CATEGORY GRADE C  
Trees of low quality

CATEGORY GRADE U  
Trees unsuitable for retention

ROOT PROTECTION AREAS (RPA)

SITE BOUNDARY

OFF SITE TREES AS RECORDED ON TOPOGRAPHICAL SURVEY

General Notes

1. The arboricultural survey is based on the supplied OSMM. This may contain inaccurate information.

2. Trees have been plotted with GPS device. The accuracy of the tree/feature location cannot be guaranteed.

3. All arrows on steps / ramps etc indicate an UP direction unless otherwise stated.

4. Contours are shown on soft detail areas only (where applicable) and annotated at the interval identified above. Hard detail areas may be contoured if specifically requested.

5. Site traffic or obstructions encountered at the time of the survey may have resulted in tree/feature features being omitted.

Survey Control

Sheet 1

| Rev    | Date | Description | CAD |
|--------|------|-------------|-----|
| Client |      |             |     |
|        |      | XXXXXXXX    |     |

ACS Consulting

ACS Consulting

Arboricultural Survey

Cross Lane

Gorton

Plotted Scale: A1@1:200

Surveyor: IRM

CAD: SPT

Checker: IRM

Rev:

Date of Issue:

July 2021

ACS Ref No: TCP/4414/Y/100